

METEODIGIT IV (9164) · Sensors



Enclosure:
Operating Instructions METEODIGIT IV (9164)

Airflow, wind speed and differential pressure measurement


The hand-held measuring instrument METEODIGIT IV and its sensors and the differential pressure module are available to measure airflow, wind speed and differential pressure.

(14433) Vane anemometer with signal generator

(14143) Vane anemometer with reed contact


An arrow on the protective ring of the vane anemometers (14143) and (14433) indicates the direction for the wind to pass through the anemometer.

Only sensor (14433): If the airflow direction is opposite to the direction indicated by the arrow, the METEODIGIT will indicate a negative wind speed.

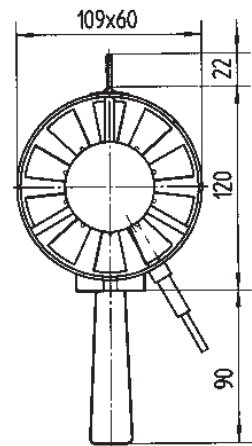

(14423) Cup rotor anemometer

The (14423) cup rotor anemometer is used to measure wind speeds of up to 90 m/s.

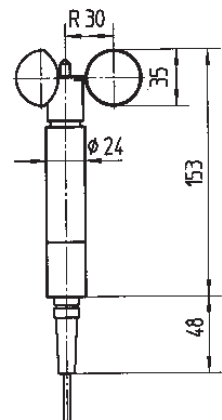

Differential pressure module

- for Pitot tubes acc. to Prandtl 0.5...40 m/s
Id-No. 32.09164.004 010
- for Pitot tubes acc. to Prandtl 1.8...90 m/s
Id-No. 32.09164.004 020

Pitot tubes according to Prandtl see manual or leaflet (628-631).



Putting into operation

After connecting the sensors to the METEODIGIT IV these are immediately operative.

Depending on the configuration 1 s- instantaneous values resp. average values over 10, 20, 30, 40, 50, 60, 70, 80, 90, 100, 110, 120 seconds will be determined.

Due to the automatic sensor recognition the METEODIGIT IV considers the starting value of the sensor. That means above the starting value each value that appears on the display now corresponds to the actual airflow or wind speed value.

Technical Data

00.14433.420 000	(14433)	Vane Generator Anemometer
Measuring element:	Measuring generator	
Measuring range:	0.4...20 m/s velocity of airflow	
Accuracy:	± 1.5 % of measuring value • ± 0.2 m/s	
Starting value:	0.4 m/s (compensated)	
Range of application:	-10...+80 °C	
Dimensions:	Protection ring outside Ø 109 mm · D 60 mm · 0.8...2 m helix cable	
Weight:	Approx. 0.4 kg	
00.14143.420 000	(14143)	Vane Reed Contact Anemometer
Measuring element:	Reed contact	
Measuring range:	0.2...20 m/s velocity of airflow	
Accuracy:	± 1.5 % of measuring value • ± 0.3 m/s	
Starting value:	0.2 m/s (compensated)	
Range of application:	-30...+150 °C	
Dimensions:	Protection ring outside Ø 109 mm · D 60 mm · 3 m cable	
Weight:	Approx. 0.4 kg	
00.14423.490 000	(14423)	Cup Anemometer
Measuring element:	Measuring generator	
Measuring range:	1.1...90 m/s wind speed	
Accuracy:	± 1.5 % of measuring value • ± 0.2 m/s	
Starting value:	1.1 m/s (compensated)	
Range of application:	-10...+80 °C	
Dimensions:	Cup Ø 65 mm · shaft Ø 23 mm · 0.8...2 m helix cable	
Weight:	Approx. 0.5 kg	

Measuring with vane anemometer (14433) and (14143)

Choice of the measuring place

In any case, a basic condition for perfect measuring results is a directed air flow without swirl at the measuring site (see DIN 1946 „VDI-Lüftungs-Regeln = VDI Ventilation Rules“).

In general such air flow conditions prevail in closed ducts having an undisturbed steadying length of $6 \times D$ (D = inside diameter of the conduit respectively equivalent diameter in case of rectangular ducts) before and $4 \times D$ behind the measuring point without sudden changes of cross section and without elbows or shut-off devices.

A steadying length of $40 \times D$ is required for measurements behind elbows. By means of suitable arranged baffles it is possible to reduce also in this case the inlet section to approx. $6 \times D$.

In case of turbulent and twisted air flow, a straightener has to be installed at a distance of approx. $1 \times D$ in front of the anemometer. This straightener can easily be assembled from a number of thin-walled tubes which should have a diameter of approx. $1/10 D$ and a length of approx. $3/10 D$. They should be installed axially into the pipe line and should completely fill the flow cross section.

When taking measurements in conduits of less than 500 mm diameter (approx. 0.2 m^2), the reduction of the cross section due to the installation of the anemometer becomes effective and there will be indicated too high velocity values.

Measurements taken in front of the air intakes and behind induction openings often have their difficulties as the velocity outside the duct decreases very quickly with the distance from the inlet. The jet cross section increases and the direction of the air flow changes simultaneously. If local conditions allow, we recommend to attach a duct piece with the same cross section at such openings and to measure the velocity within this extension. The length of the duct piece should be determined taking into consideration the above - mentioned steadying lengths. It is advisable to reduce the cross section for the purpose of shortening the extension piece, otherwise losses of pressure will occur which falsify the measuring results. Correct measuring results can be obtained within the free jet without an extension of the duct in case of large air passage at low velocity.

Measurement

In case of mobile use, an optional available handle can be screwed onto the anemometer. The handle is fastened by means of the centric M8 female thread in the base plate or of the two M5 female threads arranged on the left and right side of the M8 thread.

By using the same threads, a stationary mounting of the anemometers is possible. Before doing so it is necessary to measure the velocity profile (see later). Hereafter the instrument can be fastened at a site with mean velocity. Consequently, the anemometer is not always arranged centrally in the measuring cross section.

Vane anemometer operates independent of the position, but not independent of the flow direction. In general, they have to be held or installed in such a way that the flow reaches the vane wheel in the direction of the arrow arranged on

the protective ring. Deviations up to a maximum of 10° are permissible.

In principle it is possible to sense also return flows. In this case the polarity of the output current remains the same. If return flows shall not be sensed, a direction discriminator has additionally to be used as indicator for the direction of rotation.

Mobile measurement

In case of mobile measurements it is recommended to set the vane wheel running by blowing against it before holding it into the flow thus avoiding a too strong pulsating load.

Taking the mean

In general, the air flow velocity is not equal at all points of a duct cross section or air passage. In order to obtain exact measuring results in large cross sections it is therefore necessary to carry out a series of individual measurements the mean of which represents the actual flow velocity. Different procedures can be used in order to effect these measurements.

Grid method

The cross section redivided into the largest possible number of equal areas and one measurement is taken in the center of each such area. The mean value of all measurements is the average velocity which is decisive for the determination of the quantity of flow. The quantity of flow can also be ascertained - particularly in the case of partially covered passages - by multiplying each measured velocity value with the relevant cross sections. The sum of all individual measurements thus obtained represents the quantity of flow.

Line of gravity method

In a duct with circular cross section it is recommended to take measurements in two diameters standing vertically to each other in order to determine the mean velocity. The results are plotted graphically in relation to the diameter and the velocity profiles are plotted accordingly. The diameter should be subdivided into 5 or 10 circular rings of equal area. Now the velocities corresponding to the circles of the center of gravity of these ring areas (including the circle of the center of gravity of the central circular area) can be taken from the graph. Their arithmetic mean represents the mean velocity.

The mean velocity multiplied with the inside cross section of the duct is the quantity of air flow. The graphical representation is not required if the measurements are taken in the circles of the center of gravity.

The following table shows the radii of the center of gravity when dividing a circular cross section with the radius $r = 1$ into $n = 5$ rings (10 measuring points across the diameter) or $n = 10$ rings (20 measuring points across the diameter). The radii of the circles of the center of gravity which have to be considered when carrying out the measurement, are obtained by multiplying the gravity point radii with the actual radius of the duct.

n	Schwerpunktradien Radii of the center of gravity									
	n ₁	n ₂	n ₃	n ₄	n ₅	n ₆	n ₇	n ₈	n ₉	n ₁₀
5	0,95	0,84	0,71	0,55	0,32					
10	0,97	0,92	0,87	0,81	0,75	0,67	0,59	0,50	0,39	0,22

n = number of circular rings of equal areas

If measurements are carried out in ducts with square or rectangular cross section it is, in general, sufficient to determine only the velocity profiles of the two symmetrical axes which are perpendicular to each other and to determine their arithmetic mean as a measure of the mean velocity.

Loop measurement


In case of very wide ducts, tunnels or pits, the loop measurement will give completely satisfactory results. For this purpose, the instrument should be moved during the measuring period in serpentine or large loops having the shape of a figure 8 across the measuring cross section.

Correction in case of small measuring cross section

Vane anemometers are balanced in such a way that the named output signal is correct in such cases when the measuring value transmitters are used in a relatively large measuring cross section. When taking measurements in closed conduits of less than 500 mm. inside diameter (surface of cross section approx. 0.2 mm the reduction of the cross section due to the installation of the instrument becomes effective and there will be measured more or less too high flow velocities depending on the diameter of the tube. The actual velocity v_{tats} can then be determined from read velocity v_a , inside diameter of the tube F_R and the ideal cross section of the anemometer F_i by referring to the following formula:

$$v_{tats} = \frac{(F_R - F_i)}{F_R} * v_a$$

The anemometer has a ideal cross section $F_i = 2795 \text{ mm}^2$, if the inside diameter of tube is larger than 109 mm.

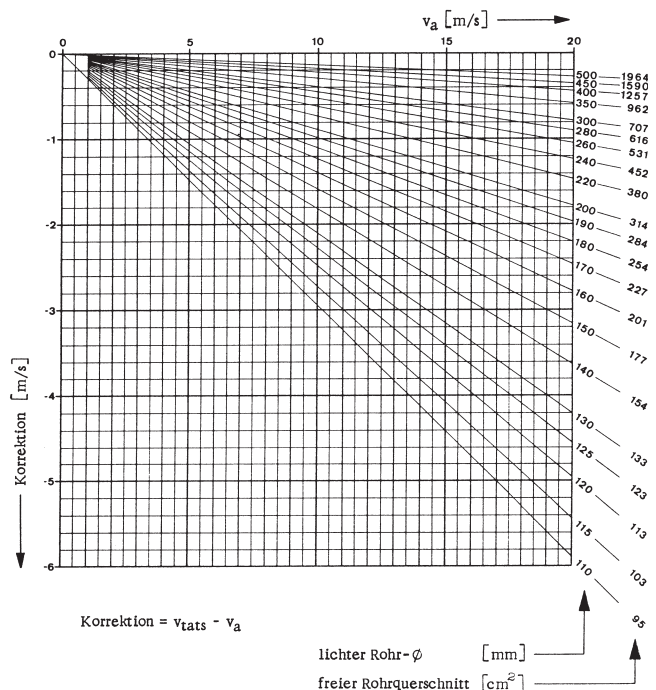


Maintenance

The vane wheel is made of a hard light metal alloy and there fore it is largely insensitive to mechanical influences. It should, however, be taken into consideration that any forceful bending of the vanes influences the original adjustment.

A cleaning of the surface of the anemometer should be carried out in dependence on the degree of contamination of the air to be tested and the frequency of use. A cleaning and re-oiling of the ball bearings of the vane wheel should not be carried out anytime by yourself, because the running qualities should be very influenced (in the extreme case, the anemometer should be destroyed).

If a significant change of the running qualities is detect, the instrument should be send to LAMBRECHT meteo GmbH for servicing.

Dimensional drawing (14433) and (14143)

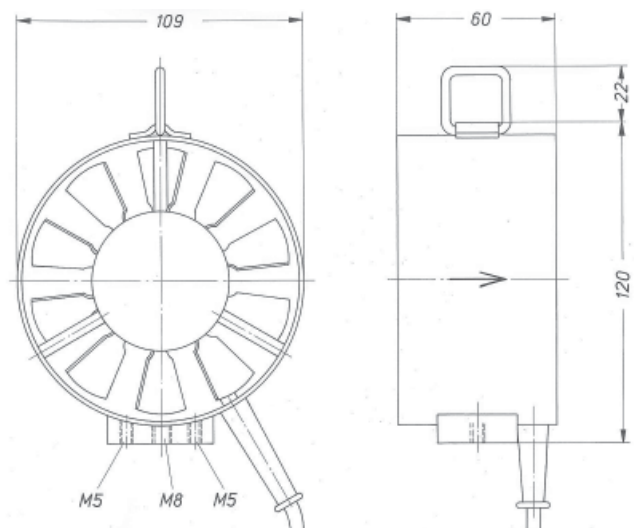

Specification	Id-No.
Hand-held measuring instrument METEODIGIT IV for airflow, wind speed, relative humidity and air temperature	00.09164.000 000
Cup rotor anemometer with measuring generator	00.14423.490 000
Vane anemometer with measuring generator	00.14433.420 000
Vane anemometer with reed contact, serviceable with maximum temperatures of 150 °C	00.14143.420 000
Differential pressure module for Pitot tubes acc. to Prandtl 0.5...40 m/s	32.09164.004 010
Differential pressure module for Pitot tubes acc. to Prandtl 1.8...90 m/s	32.09164.004 020
Accessory Adapter for mains supply	32.09164.012 000
Transport case for one METEODIGIT IV and the sensors 00.14423.490 000 or 00.14143.420 000 or 00.14433.420 000	50.09164.002 000

Please note the loss of warranty and non-liability by unauthorised manipulation of the system. You need a written permission from LAMBRECHT meteo GmbH for changes of system components. These activities must be operated by a qualified technician.

The warranty does not cover:

1. Mechanical damages caused by external impacts (e. g. icefall, rockfall, vandalism).
2. Impacts or damages caused by over-voltages or electromagnetic fields which are beyond the standards and specifications in the technical data.
3. Damages caused by improper handling, e. g. by wrong tools, incorrect installation, incorrect electrical installation (false polarity) etc.
4. Damages which are caused by using the device beyond the specified operation conditions.



Quality System certified by DQS according to
DIN EN ISO 9001:2008 Reg.No. 003748 QM08

Subject to change without notice.

09164_Sens_b-de.indd 51.16

LAMBRECHT meteo GmbH
Friedländer Weg 65-67
37085 Göttingen
Germany

Tel +49-(0)551-4958-0
Fax +49-(0)551-4958-312
E-Mail info@lambrecht.net
Internet www.lambrecht.net